



Ultra Low Vibration & Ultra High Vacuum Cryostat

The CS210°F-GMX-20B opens up a wide range of possibilities never before possible with a closed cycle cryocooler. The ARS manufactured GMX-20B interface, similar to other “B” series ARS systems is a True UHV Interface (10^{-11} Torr) where all of the rubber o-ring seals have been replaced with welded joints and metal seals. The GMX-20B interface uses a Helium Exchange Gas to decouple the sample from the cold tip of the DE210 Cryocooler. This prevents almost all vibration from being transmitted to the sample. Sample vibration levels of $<10\text{nm}$ have been demonstrated by users. Due to the exchange gas being less conductive, the base temperature will increase by 1K and the cooling capacity is roughly cut in half at varying temperatures.

Applications

- Ultra high vacuum sample environments
- Microscopy Applications
- Surface Science
- Nanomaterials
- Quantum Materials

Features


- Ultra Low Vibrations ($<10\text{ nm}$)
- True UHV (10^{-11} Torr)
- Bakeable to 200C with cold head removed
- Fully customizable
- Cold Tip Down Orientation
- UHV Compatible wiring services

Typical Configuration

- Cold head (DE-210SF)
- Compressor (ARS-10HW)
- 2 Helium Hoses
- GMX-20 Ultra Low Vibration Interface
- Nickel Plated OFHC copper radiation shield terminating 0.125” short of the cold tip
- 2 High purity quartz windows
- Instrumentation for temperature measurement and control:
 - 10 pin hermetic feed through
 - 50 ohm thermfoil heater
 - Silicon diode sensor curve matched to ($\pm 0.5\text{K}$) for control
 - Calibrated silicon diode sensor ($\pm 12\text{ mk}$) with 4 in. free length for accurate sample measurement.
- Wiring for electrical experiments:
 - 10 pin hermetic feed through
 - 4 copper wires
- Sample holder for optical and electrical experiments
- Temperature Controller

Options and Upgrades

- $<4\text{K}$ Coldhead (1.1W @ 4.2K)
- 450K High Temperature Interface
- 800K High Temperature Interface
- Manipulators & Nanopositioners
- Custom temperature sensor configuration (please contact our sales staff)
- Custom wiring configurations (please contact our sales staff)
- Window material upgrades (custom materials available)
- Sample holder upgrades (custom sample holders available)

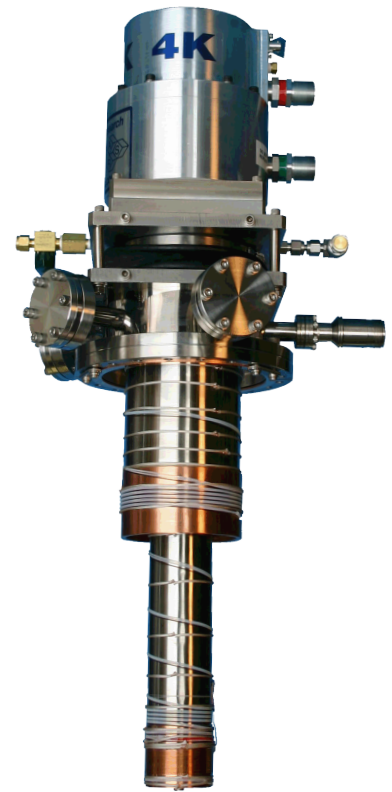

The above picture shows the DE210 Cryocooler installed on a GMX-20B interface with the radiation shield removed.



The above picture shows a standard GMX-20B cryocooler with a radiation shield.



Ultra Low Vibration & Ultra High Vacuum Cryostat

Cooling Technology

DE-210	Closed Cycle Cryocooler
Refrigeration Type	Pneumatically Driven GM Cycle
Liquid Cryogen Usage	None, Cryogen Free

Temperature* GMX-20 adds ~1K to base temperature

DE-210AF	< 9K - 350K
DE-210SFg	< 2.7K - 350K
With 800K Interface	(Base Temp + 2K) - 700K
With 450K Interface	(Base Temp + 2K) - 450K
Stability	0.1K

*Based on bare cold head with a closed radiation shield, and no additional sources of experimental or parasitic heat load

Sample Space

Diameter	61 mm (2.4 in.)
Height	39 mm (1.53 in.)
Sample Holder Attachment	1/4 - 28 screw
Sample Holder	www.arscryo.com/Products/SampleHolders.html

Optical Access

Window Ports	4 - 90° Apart
Diameter	41 mm (1.63 in)
Clear View	32 mm (1.25 in)
#/F	1.8
Window Material	www.arscryo.com/Products/WindowMaterials.html

Temperature Instrumentation and Control (Standard)

Heater	50 ohm Thermofoil Heater anchored to the coldtip
Control Sensor	Curve Matched Silicon Diode installed on the coldtip
Sample Sensor	Calibrated Silicon Diode with free length wires
Contact ARS for other options	

Instrumentation Access

Instrumentation Skirt	Bolt-On, Stainless Steel
Pump out Port	1 - NW 25
Instrumentation Ports	2
Instrumentation Wiring	Contact sales staff for options

Vacuum Shroud

Material	Aluminum
Length	388 mm (15.29 in)
Diameter	86 mm (3.38 in) at the sample space
Width	86 mm (3.38 in) at the sample space

Radiation Shield

Material	Nickel Plated OFHC Copper
Attachment	Threaded
Optical Access	0, 2, or 4 (customer specified)

Cryostat Footprint

Overall Length	787 mm (31 in)
Motor Housing Diameter	156 mm (6.14 in)

Cryocooler Model

DE-210AF



DE-210SFg

	Frequency	60 Hz	50 Hz	60 Hz	50 Hz
Base Temperature		<9K	<9K	<2.7K	<2.7K
Cooling Capacity*	4.2K	-	-	1.1W	1.1W
	10K	4W	4W	6W	6W
Radiation Shield Cooling Capacity		60W	60W	60W	60W
Cooldown Time	20K	35 min	35 min	40 min	40 min
	Base Temperature	70 min	70 min	80 min	80 min
Compressor Model		ARS-10HW		ARS-10HW	
Typical Maintenance Cycle		12,000 hours		12,000 hours	


Understanding the GMX-20 Interface

The X-20 Interface uses a Helium Exchange Gas to decouple the sample space from the cold tip of the cryocooler. This prevents almost all vibration from being transferred to the sample space. **Current measurements with the GMX-20-OM Interface indicate +/- 5 nanometers at the sample.**

1. The Cryocooler is supported from a Floor Stand
2. The soft rubber bellows minimize vibrations transmitted to the sample while keeping in the Helium Exchange Gas.
3. The cold tip has 10-30 micron vibrations (depending on CCR model) but no direct contact with the sample space.
4. Convective pockets of Helium Exchange Gas cools the sample space.
5. The sample is only in contact with the X-20 Interface
6. The X-20 Interface is mounted directly on a (user provided) Vibration Isolation Table.

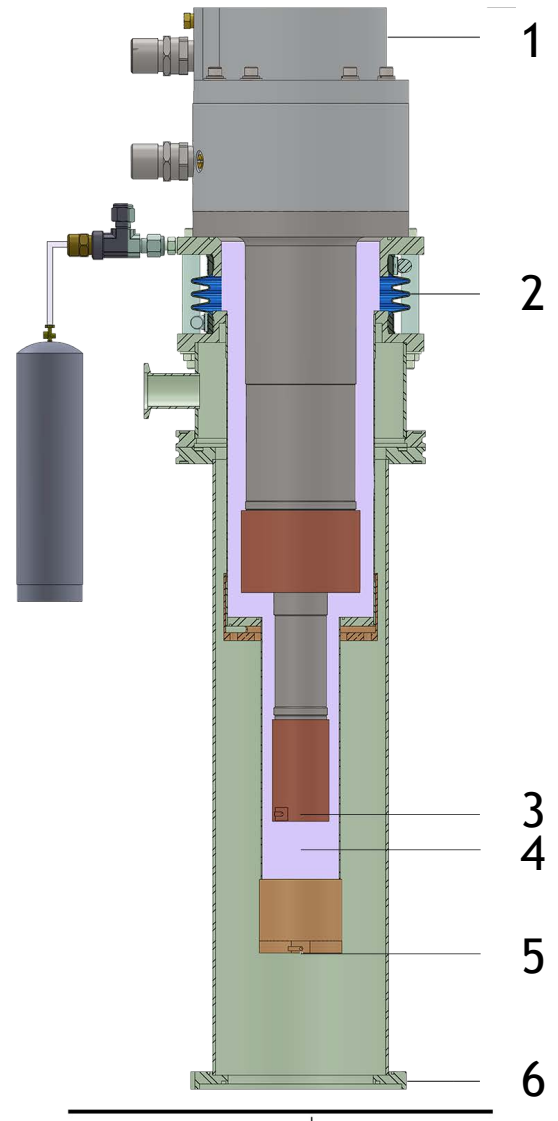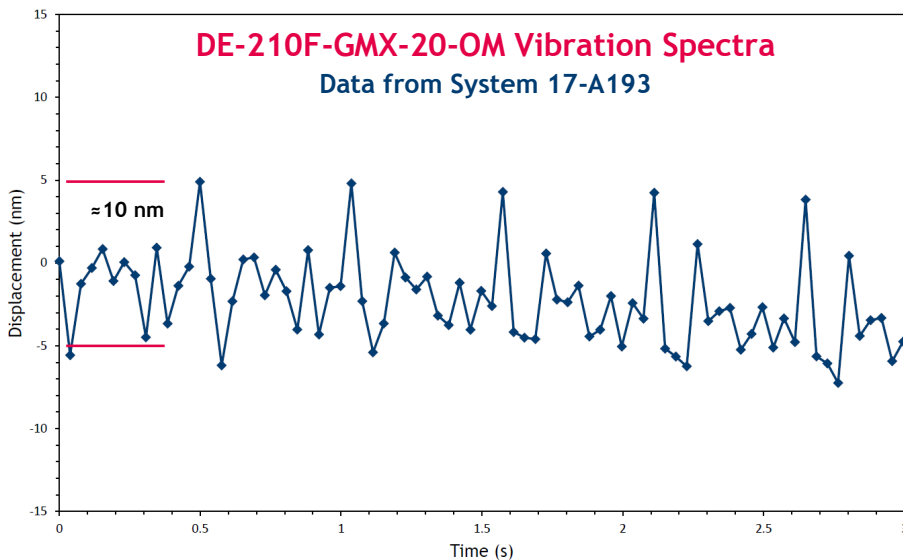

DE210*F-GMX-20 Outline Drawing

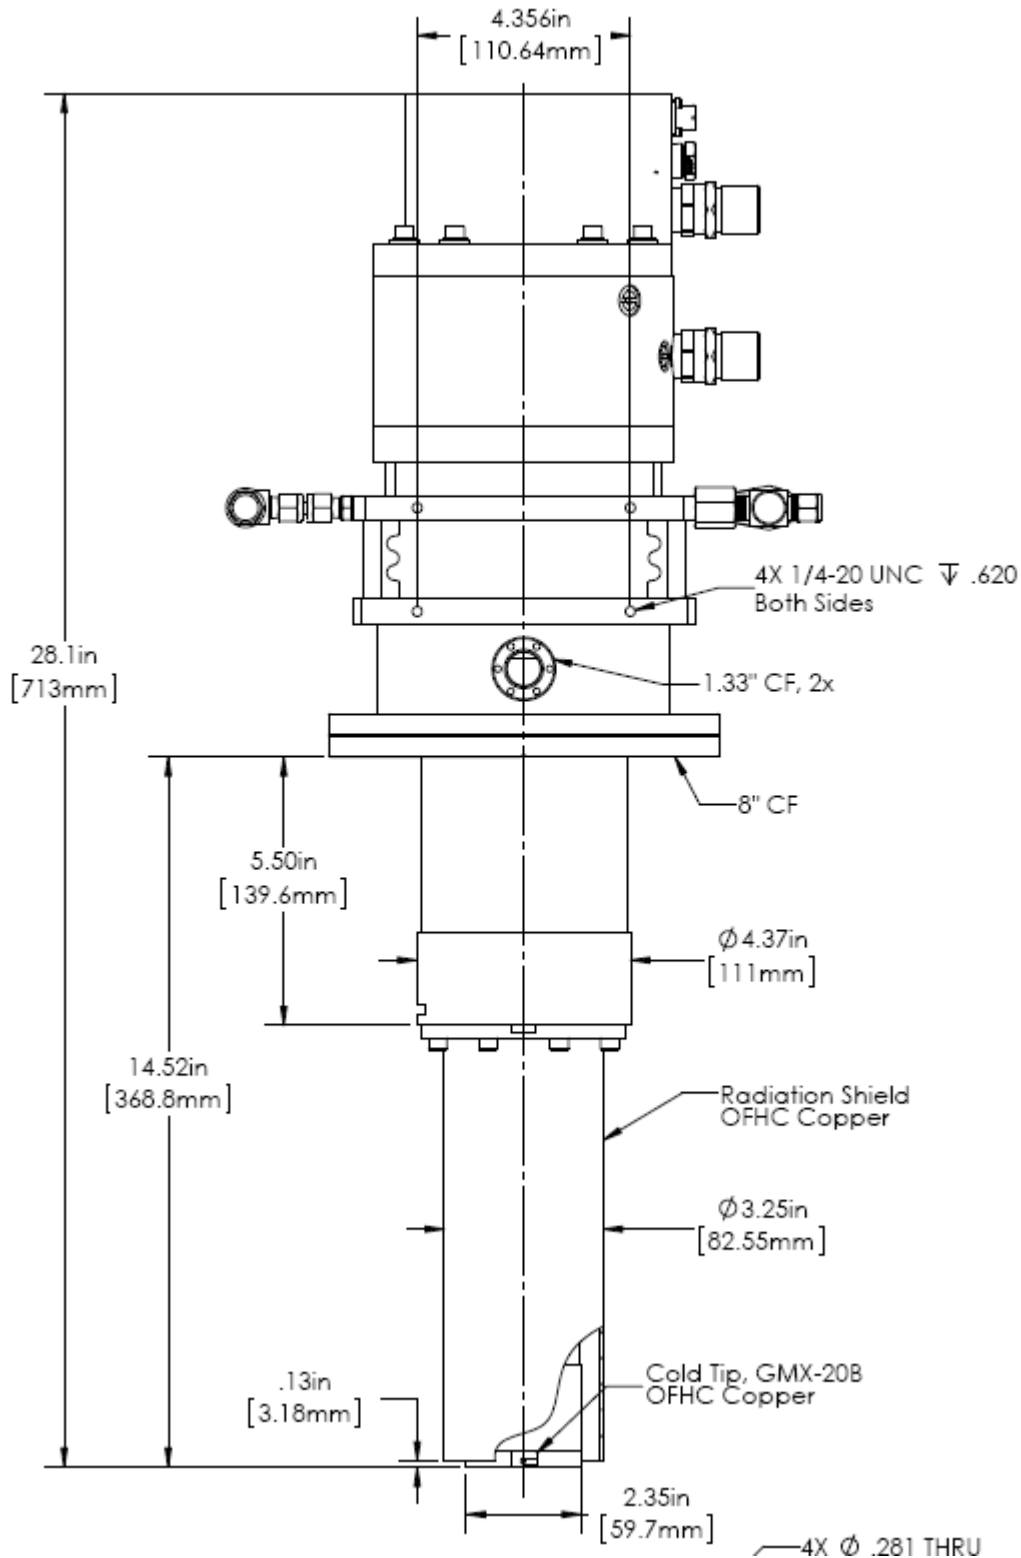




Ultra Low Vibration & Ultra High Vacuum Cryostat

Direct Mounting




The DMX-20 can be direct mounted on the Cryocooler. The vibrations at the sample will go up to 140 nm. It can be useful if the sample has to be translated in XYZ.

ARS-10HW Compressor

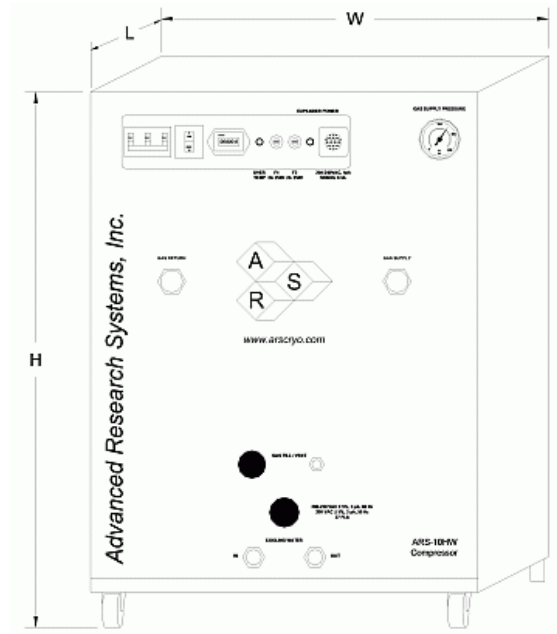

Floor Stand

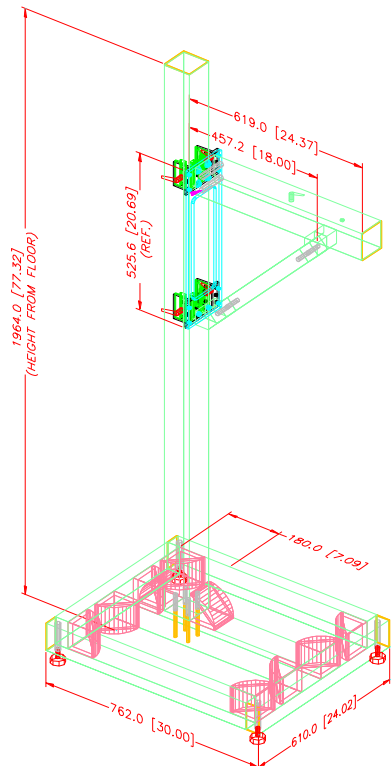


Compressor Model

ARS-10HW

	Frequency	60 Hz, 3 Phase	50 Hz, 3 Phase
Standard Voltage	Min	208 V	190 V
	Max	230 V	210 V
High Voltage	Min	380 V	440 V
	Max	415 V	480 V
Power Usage	Three Phase	6.8 kW	6.8 kW
Refrigerant Gas		99.999% Helium Gas, Pre-Charged	
Ambient Temperature		5 - 40 C (40–104 F)	
Cooling Water	Consumption	5.7 L / min (1.5 Gal. / min)	
	Temperature	< 20 C (68 F)	
	Connection	1/2 in. Swagelok Fitting	
Dimensions:	L	483 mm (19 in)	
	W	533 mm (21 in)	
	H	617 mm (24.3 in)	
Weight		105 kg (230 lbs)	
Typical Maintenance Cycle		12,000 hours	

Mossbauer Spectra with DMX-20

Cryocooler Off

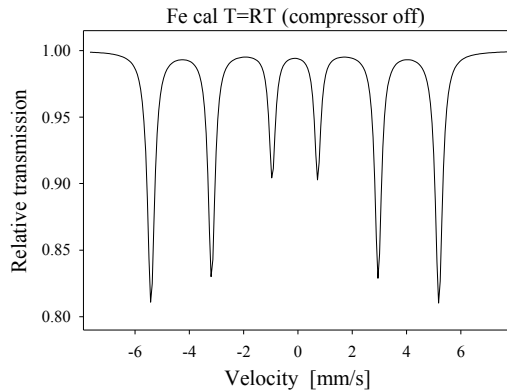

Calculated parameters:

WID=0.269 mm/s

W13=1.17

W23=1.08


ISO=0.000 mm/s

BHF=32.94T

Calibration spectrum:

Measurement with metallic iron foil (thickness 25 mm)

Cryocooler On

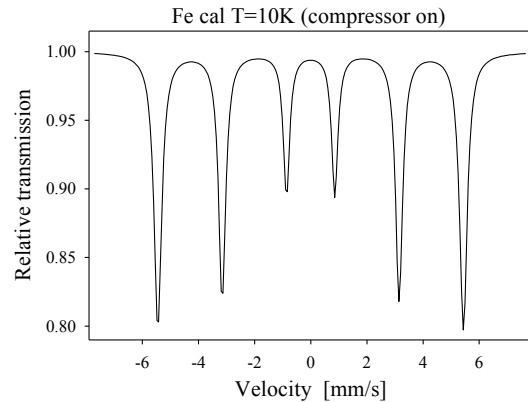

Calculated parameters:

WID=0.270 mm/s

W13=1.21

W23=1.11

ISO=+0.115 mm/s

BHF=33.81T

Calibration spectrum:

Measurement with metallic iron foil (thickness 25 mm)

When the system is properly mounted to the wall and the table and properly adjusted then the effect of vibrations induced by the working compressor is very small (almost negligible).

and The broadening (rather no broadening!) is fully reproducible is well below 2%. Such broadening has practically no effect and in almost all cases can be ignored. However, compare the linewidths calculated in the same way!


The Displex system is virtually vibration free!

Prof. Dr. habil. Michal Kopcewicz

Institute of Electronic Materials Technology


WARSAW, Poland

Mossbauer Cryostat, DMX-20

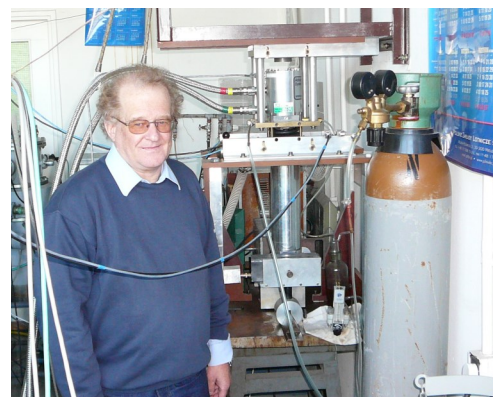

Prof. Dr. habil. Michal Kopcewicz

Possible Mossbauer Configuration

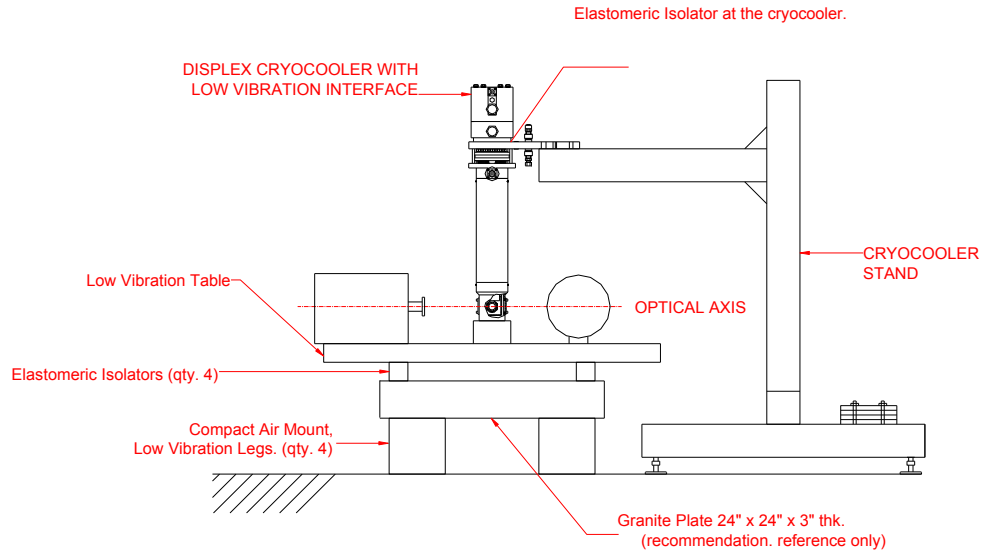


For maximum isolation proper mounting of the system is important. ARS offers a special ULV stand to isolate the ultra low vibration cryostat from the vibrating components of the cooler and the floor vibrations.

The cryocooler stand can be adjusted for the proper height, this holds the cooler.


The cryostat is mounted on the low vibration table, which consists of a high mass granite block (User supplied), resting on 4 air legs (optional ARS offering). Additional elastomeric isolators additional filter the unwanted frequencies from the floor to the cryostat.

System can be tested by shutting off the cryocooler only and watching the vibration effect on the experiment.

Ellipsometry

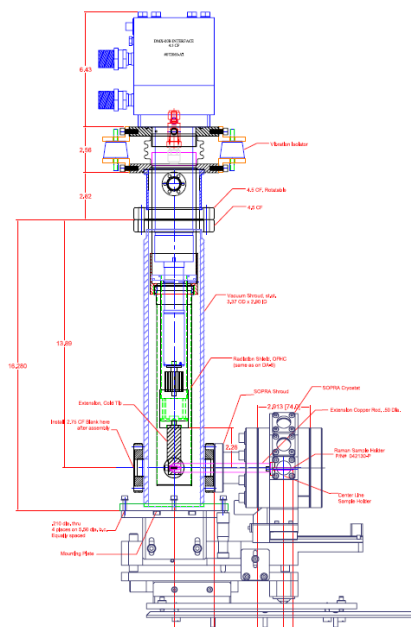

SEM Setup

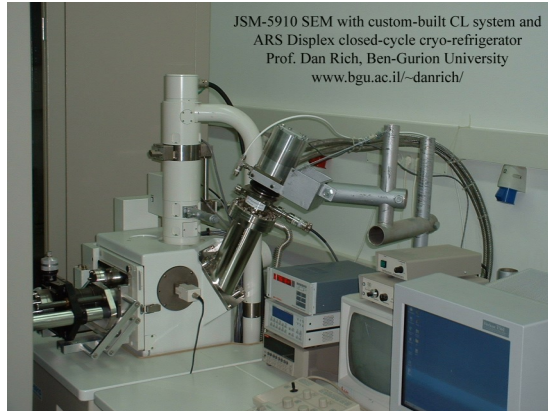

The picture shows the Displex and its interface. All items showing stainless steel in the photo are modifications to our JSM-5910 SEM. Please also note the published papers on my website, which demonstrate CL results that were acquired with this cooling system.

The sample temperature, is between 40 K and 50 K.

Courtesy; Prof. Dan Rich, Ben Gurion University, Beer Sheva, Israel.


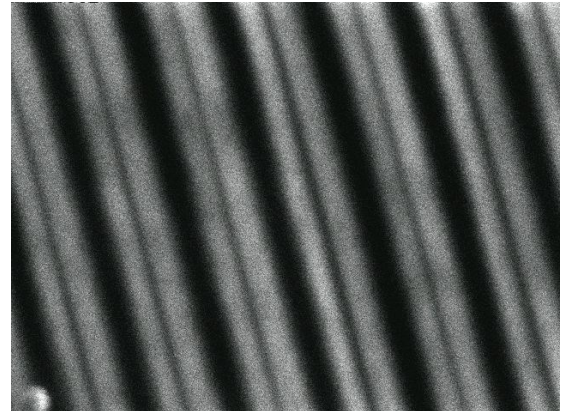


Image of a InGaN/GaN quantum well grown on a patterned GaN substrate. The patterning consists of stripes with a periodicity of 10 microns.

Monochromatic CL image (Mag. 2000) taken with a 390 nm detection wavelength.

The degradation of image quality from room temperature and 50K suggests that the vibration is less than 10nm.

FTIR Setup

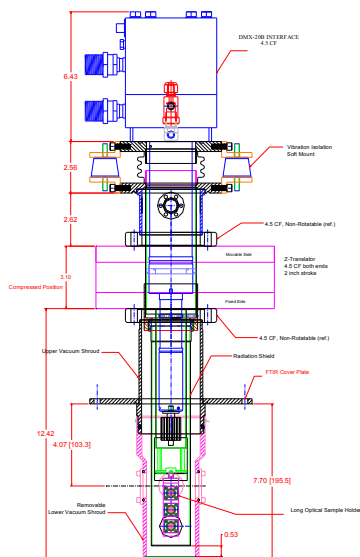

Low Vibration system for FTIR spectrometer. Sample holder with 3 samples can be translated in Z direction.




Low Vibration system for BOMEM, DA8 FTIR spectrometer.



Ultra Low Vibration & Ultra High Vacuum Cryostat


Magneto Electrical Experiments

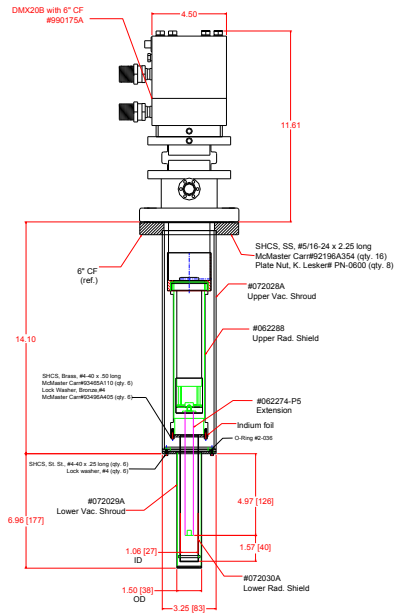

The vacuum shroud becomes narrow to permit sample insertion into a small magnet pole space.

The vacuum shroud becomes narrow to permit sample insertion into a small magnet pole space.

Magneto Optical Experiments (MOKE)

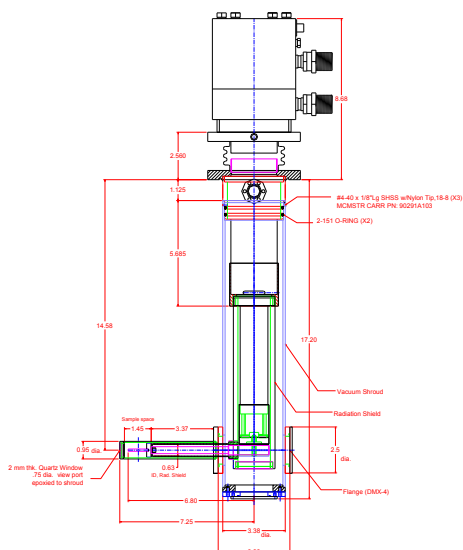

Low Vibration Side looking window can be placed in a MOKE, (Magneto Optical Kerr Effect). Sample can be located in any plane. The pole spacing can be as low as 1 inch.

Small diameter vacuum housing can be inserted into a narrow gap (high field). The optical window allows collection of light from the sample. The window can be very close to the sample for short focal length objective.